

Biofeedback by using Electrical Stimulation (Prof. Dr H. Yokoi)

Man-machine interfaces are leading into an era where the intelligent devices are becoming part of our every day lives. In our laboratory we work in the development and implementation of a biofeedback interface for an electrically powered electromyography (EMG) controlled prosthetic hand (Fig.1). One of the major problems for the prosthetic devices is the lack of feedback to the human body that will help in the recognition of the device, facilitating its control. Having only visual feedback, and lacking of any form of proprioception, the prosthetic's users requires of a conscious effort in order to control the prosthesis.

Providing with an interface that allows the user to interact directly with the device will increase its controllability. In our laboratory we use functional electrical stimulation (FES) (Fig 2) to supply the user with tactile information by translating pressure into electrical stimulation. In the current development, we use conductive rubber based pressure sensors that provide the interaction between surrounding environment and the machine. The signal acquired is then translated into a duty cycle controlled pulse based stimulation signal to interact with the human body. We expect that the biofeedback signal applied directly to the system's user will allow the subject to have direct interaction with the environment, reduce the effort generated by the use of only visual feedback, and increase the acceptance rate in the prosthetic hand use. Our research also includes the measurement of the biofeedback effects using fMRI (Figure 3)

Keywords: EMG control, Biofeedback, subconscious control, extended proprioception.

References

- 1) Alejandro Hernandez Arieta, Wenwei Yu, Hiroshi Yokoi, Tamio Arai: FES as Biofeedback for an EMG Controlled Prosthetic Hand, Proceedings Tencon'05 conference of the IEEE Region 10.(TENCON05), 49, (2005)
- 2) Alejandro Hernandez Arieta, Hiroshi Yokoi, Takashi Ohnishi, and Tamio Arai: An f-MRI Study of an EMG Prosthetic Hand Biofeedback System, Intelligent Autonomous Systems 9, IOS Press, ISBN 1-58603-595-9, pp.921-929, (2005)
- 3) Alejandro Hernandez Arieta, Wenwei Yu, Hiroshi Yokoi, Tamio Arai: Study on the Effects of Electrical Stimulation on the Pattern Recognition for an EMG Prosthetic Application, Proc. of the 27th annual International Conference of the IEEE Engineering In Medicine and Biology Society (EMBS05), 280 (2005)
- 4) Hiroshi Yokoi, Alejandro Hernandez Arieta, Ryu Katoh, Wenwei Yu, Ichiro Watanabe, Masaharu Maruishi: Mutual Adaptation in a Prosthetics Application, Embodied Artificial Intelligence edited by Fumiya Iida, Rolf Pfeifer, Luc Steels, and Yasuo Kuniyoshi, LNCS/LNAI series of Springer, Springer (published in 2004).
- 5) Prosthetic hand control with tactile sensory feedback. 2003 JSME Conference on Robotics and Mechatronics. (ROBOMECH03) 2P2-3F-A7, 2003
- 6) Alejandro Hernandez Arieta, Wenwei Yu, Hiroshi Yokoi et al. Integration of a Multi-D.O.F. Individually Adaptable EMG Prosthetic System with Tactile Feedback. IAS-8, F.Groren et al.(Eds) IOS Press, pp.1013-1021,(2004).



Fig. 1 EMG controlled Prosthetic Hand




Fig. 2 Electrical Stimulation Electrodes

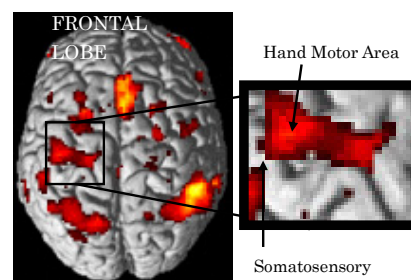


Fig. 3 Stimulation "Ilusion" (fMRI)